Order online now!

www.rockland.com
tech@rockland.com
+1 484.791.3823

Datasheet for 009-0105

Human IgG Fab

Overview

Description:	Human IgG Fab Fragment - 009-0105
Item No.:	009-0105
Size:	2 mg
Applications:	SDS-PAGE, Biochemical Assay
Origin:	Human

Product Details

Background:	Secreted as part of the adaptive immune response by plasma B cells, immunoglobulin G constitutes 75% of serum immunoglobulins. Immunoglobulin G binds to viruses, bacteria, as well as fungi and facilitates their destruction or neutralization via agglutination (and thereby immobilizing them), activation of the compliment cascade, and opsonization for phagocytosis. The F(ab) fragment is the portion of the antibody that binds to the antigen target. The immunoglobulin Fab also possesses one constant and one variable region of both the heavy and light chain.
Synonyms:	Human Immunoglobulin Fab, F(ab), Fragment antigen-binding
Species of Origin:	Human
Format:	IgG Fab
Type:	Native Protein

Target Details

Purity/Specificity:	Human IgG Fab fragment was prepared from normal serum by a multi-step process which includes delipidation, salt fractionation and ion exchange chromatography followed by papain digestion and extensive dialysis against the buffer stated above. Human IgG Fab fragment assayed by immunoelectrophoresis resulted in a single precipitin arc against anti-Human Serum, anti- Human IgG and anti- Human IgG F(ab')2. No reaction was observed against anti- Human IgG F(c) or anti-Papain.
Relevant Links:	• 009-0105 SDS

Application Details

Tested Applications:	SDS-PAGE
Suggested Applications:	Biochemical Assay (Based on references)
Application Note:	Human IgG Fab Fragment has been tested in SDS-Page and can be utilized as a control or standard reagent in Western Blotting and ELISA experiments.
Assay Dilutions:	All assays should be optimized by the user. Recommended dilutions (if any) may be listed below.


Formulation

Physical State:	Liquid (sterile filtered)
Concentration:	2 mg/mL by UV absorbance at 280 nm
Buffer:	0.02 M Potassium Phosphate, 0.15 M Sodium Chloride, pH 7.2
Preservative:	0.01% (w/v) Sodium Azide
Stabilizer:	None

Shipping & Handling


Shipping Condition:	Wet Ice
Storage Condition:	Store vial at 4° C prior to opening. This product is stable for several weeks at 4° C as an undiluted liquid. Dilute only prior to immediate use. For extended storage, aliquot contents and freeze at -20° C or below. Avoid cycles of freezing and thawing.
Expiration:	Expiration date is one (1) year from date of receipt.

Images

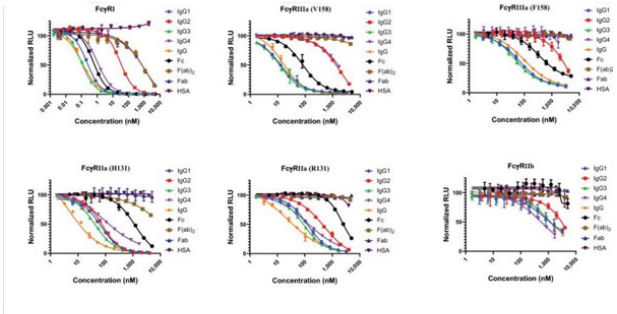


	IgG1	IgG2	IgG3	IgG4	IgG	Fc
FcγRI	0.23	29.40	0.09	1.07	0.11	0.56
FcγRIIa (H131)	67.04	77.12	40.78	102.20	4.64	1198.00
FcγRIIa (R131)	122.30	518.80	85.03	127.50	25.81	2284.00
FcγRIIb*	n.d.	n.d.	819.30	573.10	988.80	n.d.
FcγRIIIa (V158)	12.33	2045.00	12.28	n.d.	15.70	81.04
FcγRIIIa (F158)	65.04	n.d.	44.80	n.d.	99.39	342.30


Figure
Dose dependent inhibition curves generated with six different FcγR assays. Four different set of samples were tested to show the specificity and subclass specific binding. Analytes tested are (1) human IgG subclasses IgG1, IgG2, IgG3, IgG4; (2) human IgG; (3) Fc, Fab, and F(ab)2 domains; and (4) human serum albumin (HSA). Data represent the mean ± standard error of triplicate experiments. IC50 (nM) values calculated from the inhibition curves are shown in the Table. IC50 values are in nM. *For FcγRIIb IC50 values are intended only for qualitative purposes as mentioned in the text. n.d. not determined. Figure 3. PMID: 35842448.

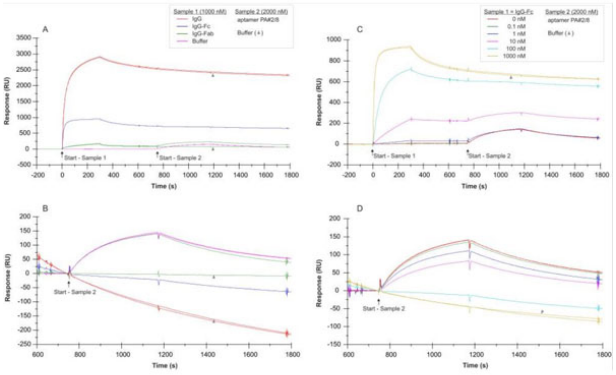

Surface Plasmon Resonance (SPR)
SPR interaction analyses regarding the aptamer binding site in Protein A.Biacore X100 / sensor chip CAP / ligand: biotinylated Protein A with immobilization level of ~560 RU / two-step analyte binding without regeneration in between, (A-B) analyte 1 = sample 1: human IgG, IgG-Fc fragment, IgG-Fab fragment with a concentration of 1000 nM each, or buffer, (C-D) analyte 1 = sample 1: concentration series of human IgG-Fc in the range of 0–1000 nM, (A-D) analyte 2 = sample 2: 2000 nM 5'-fluorescein-labeled aptamer PA#2/8 or buffer. Double-referenced sensorgrams are shown (blank reference surface without Protein A, buffer injection). Binding of sample 1 followed by sample 2 is shown in (A) and (C) with alignment to injection start of sample 1. In (B) and (D) only binding of sample 2 with alignment to injection start of sample 2 is shown. Fig 12. PMID: 26221730.

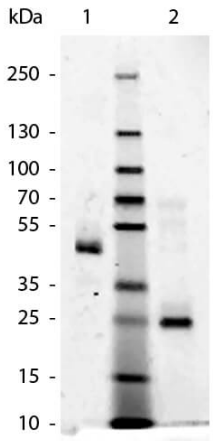

SDS-PAGE
SDS-Page of Human Fab. Lane 1: Human Fab - Non-Reduced. Lane 2: Human Fab - Reduced. Load: 1.0 ug per lane. Predicted/Observed size - Non-Reduced: 50 kDa, 50 kDa for Human Fab. Predicted/Observed size - Reduced: 25 kDa, 25 kDa for Human Fab. Other band(s): None.

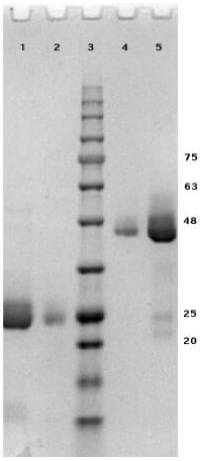

SDS-PAGE
SDS-PAGE results of Human IgG Fab Fragment. Lane 1: reduced Human IgG Fab Fragment (5ug). Lane 2: reduced Human IgG Fab Fragment (1ug). Lane 3: Opal Prestained Molecular Weight Ladder (p/n MB-210-0500). Lane 4: non-reduced Human IgG Fab Fragment (1ug). Lane 5: non-reduced Human IgG Fab Fragment (5ug). 4-20% Lonza SDS-PAGE; Coomassie Stained; BioRad ChemiDoc Imaged.

References

- Huang C et al. Age-independent anti-angiogenic therapy for choroidal neovascularization by targeting secretogranin III. *Geroscience.* (2026)
- Chanakul W et al. Large and Stable Nanopores Formed by Complement Component 9 for Characterizing Single Folded Proteins. *ACS Nano.* (2025)
- Nath, N et al. A homogeneous bioluminescent immunoassay for parallel characterization of binding between a panel of antibodies and a family of Fcγ receptors. *Scientific Reports* (2022)
- Stoltenburg, R et al. In vitro Selection and Interaction Studies of a DNA Aptamer Targeting Protein A. *PloS One* (2015)

Disclaimer

No test method can provide total assurance that the hepatitis B virus, hepatitis C virus, human immunodeficiency virus, or any other infectious agents are absent. Thus, all blood products, including purified proteins derived from human blood sources, should be handled at Biosafety Level 2 as recommended by the CDC\NIH manual entitled Biosafety in Microbiological and Biomedical Laboratories for potentially infectious human serum, blood specimens or proteins derived from same. Source material for the human blood product supplied to your facility has been tested for the detection of HIV antibody, Hepatitis B surface antigen, antibody to Hepatitis C, HIV 1 antigen(s), antibody to HTLV - I/II, and syphilis by FDA guidelines. All units were found to be non-reactive/negative for these tests. All human blood source material is collected in FDA licensed centers and is tested with FDA approved test kits.

This product is for research use only and is not intended for therapeutic or diagnostic applications. Please contact a technical service representative for more information. All products of animal origin manufactured by Rockland Immunochemicals are derived from starting materials of North American origin. Collection was performed in United States Department of Agriculture (USDA) inspected facilities and all materials have been inspected and certified to be free of disease and suitable for exportation. All properties listed are typical characteristics and are not specifications. All suggestions and data are offered in good faith but without guarantee as conditions and methods of use of our products are beyond our control. All claims must be made within 30 days following the date of delivery. The prospective user must determine the suitability of our materials before adopting them on a commercial scale. Suggested uses of our products are not recommendations to use our products in violation of any patent or as a license under any patent of Rockland Immunochemicals, Inc. If you require a commercial license to use this material and do not have one, then return this material, unopened to: Rockland Inc., P.O. BOX 5199, Limerick, Pennsylvania, USA.